ASCON spa

ISO 9001
Certified

Indicator - Transmitter Strain Gauge Input for Melt Pressure & Load Cell Transducers 1/8 DIN - 96x48

J5 line

S E R I E S


User Manual • M.I.U.J5 - 0/08.08 • Cod. J30-478-1AJ5 E



ASCON spa
via Falzarego, 9/11
20021 Baranzate
(Milano) Italy
Fax +39-02-3504243
www.ascon.it
support@ascon.it

ASCON CORPORATION
1884 East Fabyan Parkway
Batavia, Illinois 60510
Tel. +1-630-482-2950
Fax +1-630-482-2956
www.asconcorp.com
info@asconcorp.com

Indicator - Transmitter
Strain Gauge Input for
Melt Pressure &
Load Cell Transducers
1/8 DIN - 96x48
J5 line

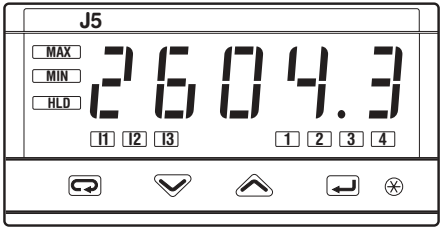

CE

NOTES ON ELECTRIC SAFETY AND ELECTROMAGNETIC COMPATIBILITY

Please read these instructions carefully before proceeding with the installation of the controller.
Class II instrument, rear panel mounting.

This indicator has been designed in compliance with:
Regulations on electrical apparatus (appliance, systems and installations) according to the European Community directive 73/23/EEC amended by the European Community directive 93/68/EEC and the Regulations on the essential protection requirements in electrical apparatus EN61010-1 : 93 + A2:95.


Regulations on Electromagnetic Compatibility according to the European Community directive #89/336/EEC, amended by the European Community directive #92/31/EEC, 93/68/EEC, 98/13/EEC and the following regulations:

Regulations on RF emissions	
EN61000-6-3 : 2001	residential environments
EN61000-6-4 : 2001	industrial environments
Regulation on RF immunity	
EN61000-6-2 : 2001	industrial equipment and system

It is the responsibility of the installer to ensure compliance with the regulations on safety requirements and EMC.
The device has no user serviceable parts and requires special equipment for repair.
For service or repair, contact the manufacturer or your sales representative.

All the information and warnings about safety and electromagnetic compatibility are marked with the ⚠CE sign, at the side of the note.

TABLE OF CONTENTS

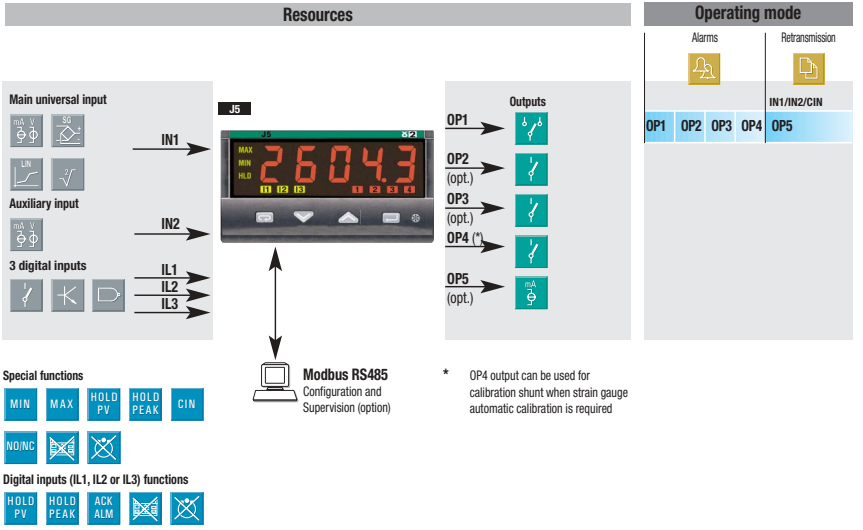

* OP4 output can be used for calibration shunt when strain gauge automatic calibration is required

1 INSTALLATION ..... Page 4
2 ELECTRICAL CONNECTIONS ..... Page 8
3 PRODUCT CODING ..... Page 14
4 OPERATION ..... Page 18
5 DISPLAYS ..... Page 34
6 COMMANDS ..... Page 35
7 TECHNICAL SPECIFICATIONS ..... Page 37

INSTALLATION


Installation must be carried out only by qualified personnel.

Before proceeding with the installation of this indicator read the instructions in this manual with particular attention to the installation precautions marked with the ⚠CE symbol.


⚠CE

To prevent contact with parts that may be electrically live, **the indicator must be installed in an enclosure.**


1.1 GENERAL DESCRIPTION

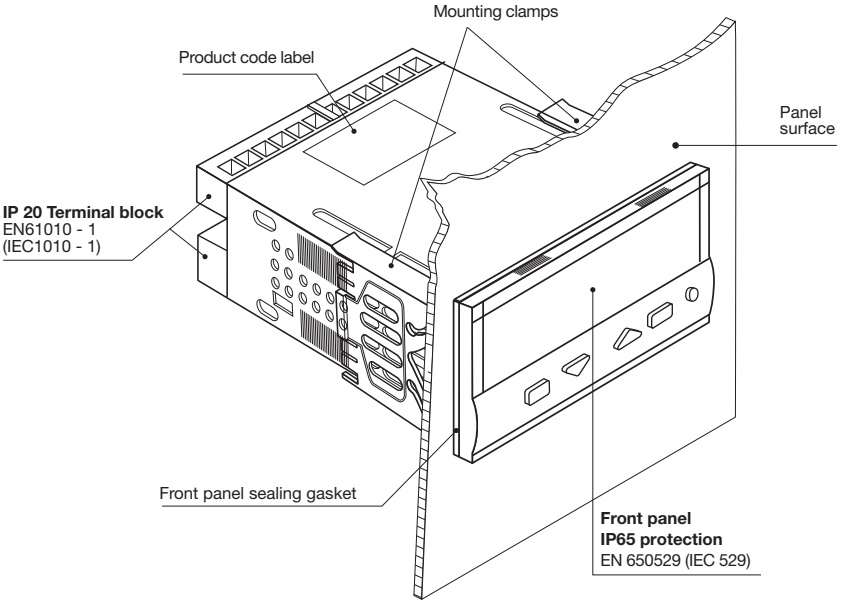

1.2 DIMENSIONS

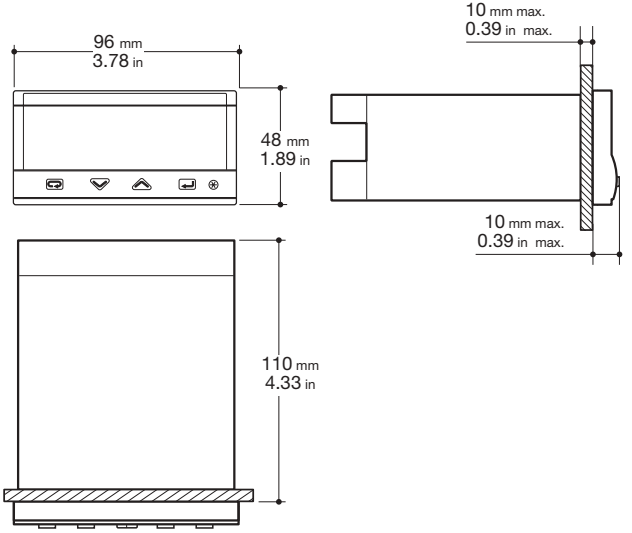

1.3 PANEL CUTOUT

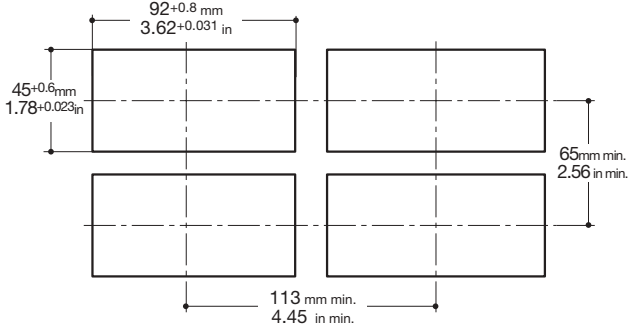

1.4 ENVIRONMENTAL CONDITIONS

Operating conditions	
	Altitude: up to 2000 m
	Temperature: 0…50°C
%Rh	Relative humidity: 5…95 % non-condensing


Special conditions		Suggestions
	Altitude: > 2000 m	Use 24Vac supply version
	Temperature: >50°C	Use forced air ventilation
%Rh	Humidity: > 95 %	Warm up
	Conducting atmosphere	Use filter

Prohibited Conditions	
	Corrosive atmosphere
	Explosive atmosphere

1.5 PANEL MOUNTING [1]


1.5.1 INSERT THE INSTRUMENT

1 Prepare panel cutout
2 Check front panel gasket position
3 Insert the instrument through the cutout

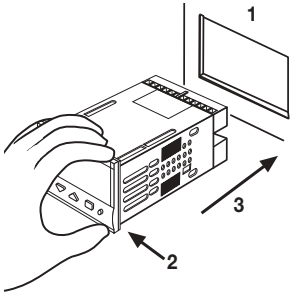


1.5.2 INSTALLATION SECURING

1 Attach the mounting clamps as shown
2 Push the mounting clamps toward the panel surface to secure the instrument




1.5.3 CLAMP REMOVAL

1 Insert the screwdriver in the clips of each clamp
2 Rotate the screwdriver




1.5.4 INSTRUMENT REMOVAL

1 Push and ...
2 Pull forward to remove the instrument

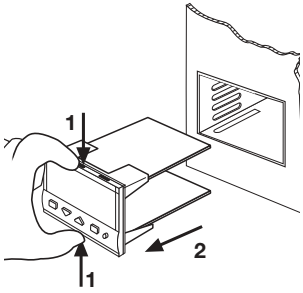


Electrostatic discharges can damage the instrument.
Before removing the instrument, the operator must discharge himself to ground.




UL note
[1] For Use on a Flat Surface of a Type 2 and Type 3 'raintight' Enclosure.

2

ELECTRICAL CONNECTIONS

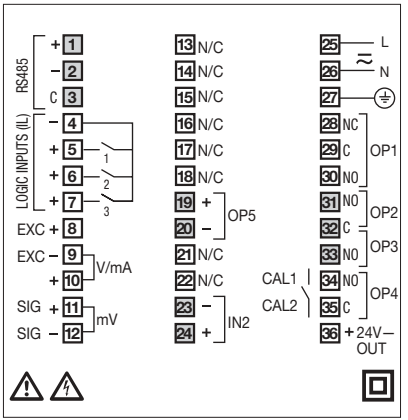

2.1 TERMINAL BLOCK [1]

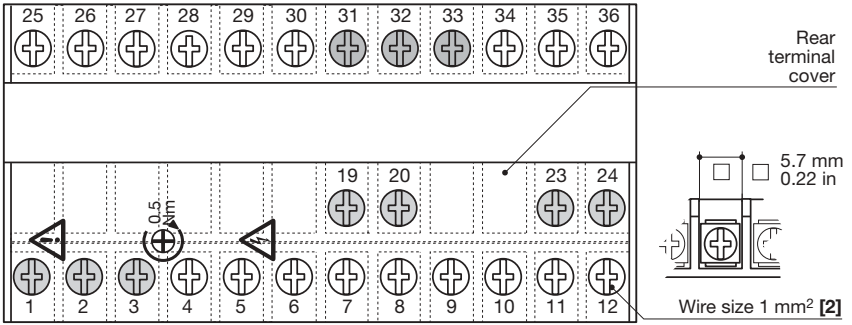

	28 screw terminals M3
	Option terminals
	Tightening torque 0.5 Nm
	Phillips screw-driver PH1
	Flat head screw-driver 0.8 x 4 mm

Terminals

	Pin connector Ø 1.4 mm 0.055 in max.
	Fork-shape AMP 165004 Ø 5.5 mm - 0.21 in
	Stripped wire L 5.5 mm - 0.21 in

UL note

[1] Use 60/70 °C copper (Cu) conductor only.

[2] Wire size 1 mm² (18 AWG Solid/Stranded)

PRECAUTIONS


This instrument has been designed to work in harsh and noisy environments (level IV of the industrial standard IEC 801-4). It is recommended to follow these suggestions.

⚠


All the wiring must comply with local regulations.
The supply wiring should be routed away from the power cables.
Avoid using electromagnetic contactors, power relays, and high power motors in close proximity.
Avoid power units in close proximity, especially if controlled in phase angle mode.

Keep low level sensor input wires away from the power lines and output wires.
If this is not possible, use shielded cables on the sensor input, with the shield connected to ground.

2.2 SUGGESTED WIRE ROUTING

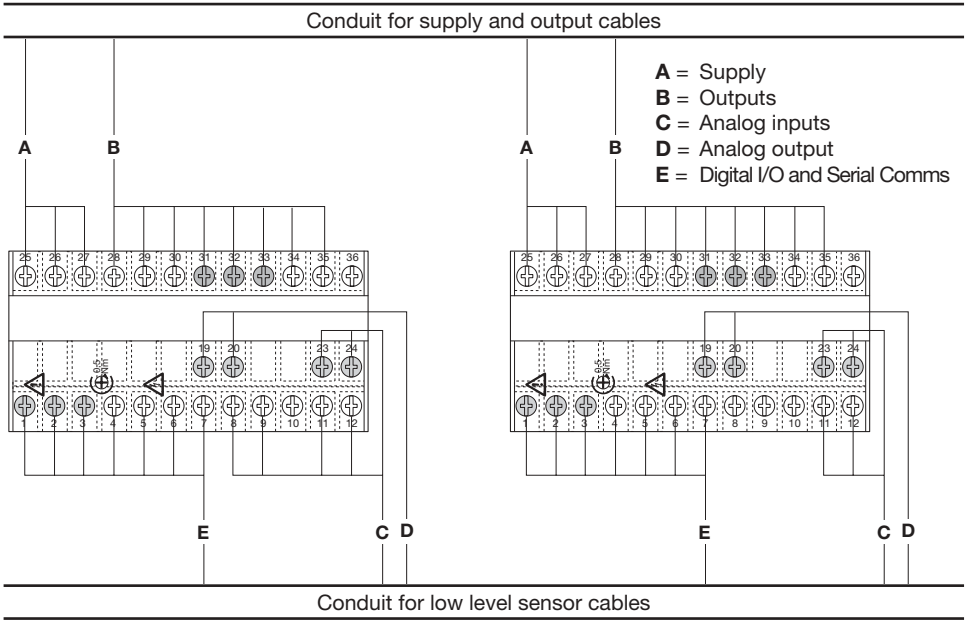

2.3 EXAMPLE OF WIRING DIAGRAM

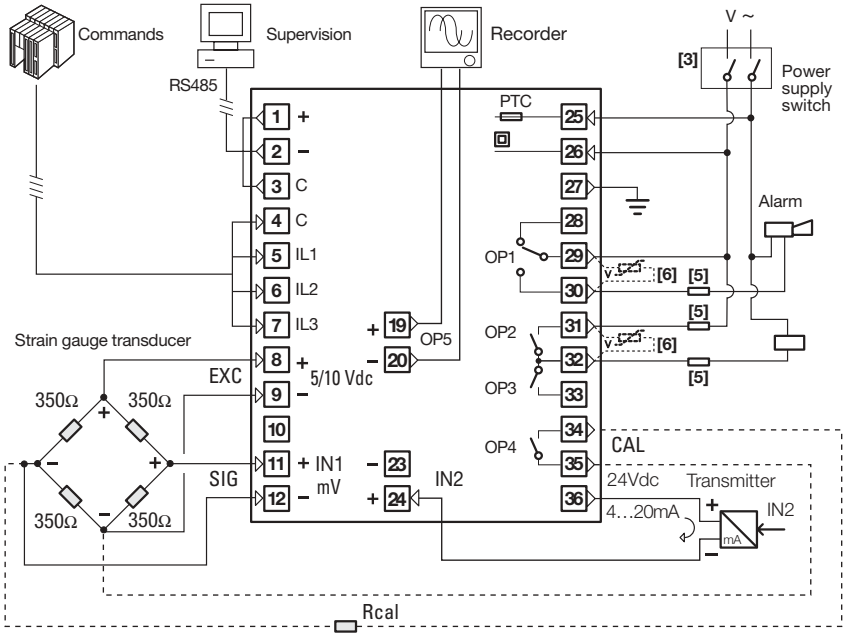

Notes:

1] Make sure that the power supply voltage is the same as indicated on the instrument label.

2] Switch the power supply on only after all electrical connections have been completed.

3] In accordance with safety regulations, install a circuit breaker on the instrument power supply line that is clearly identified for the instrument (or group of instruments). The breaker shall be easily accessible by the operator.

4] The instrument is PTC protected. In case of failure, return the instrument to the manufacturer for repair.


5] To protect the internal circuits of the instrument, use:
- 2 AT fuse for Relay outputs (220 Vac);
- 4 AT fuse for Relay outputs (110 Vac);
- 1 A acT fuse for Triac outputs.

6] Relay contacts are already protected with varistors.
Only in case of 24 Vac inductive loads, use model A51-065-30D7 varistors (on request)

2.3.1 POWER SUPPLY

Switching power supply with multiple isolation and internal PTC protection.


- **Standard version:**
  nominal voltage:
  100...240Vac (-15...+10%)
  Frequency 50/60Hz
- **Low Voltage version:**
  Nominal voltage:
  24Vac (-25...+12%)
  Frequency 50/60Hz
  or 24Vdc (-15...+25%)



For better protection against noise, it is recommended to not connect the ground clamp provided for domestic installations.


2.3.2 MAIN INPUT (IN1)

A1 For mV



A2 4 wire Strain Gauge Input

- Set code L = 1 or 2 (see page 16) to obtain 5 or 10 Vdc stabilized power supply for the external strain gauge bridge, terminals 8 (+) and 9 (-).
- Set code I = 0, 1 or 2 (see page 16) to obtain suitable mV input (20,520 or 100 mV), terminals 11 (+) and 12 (-).

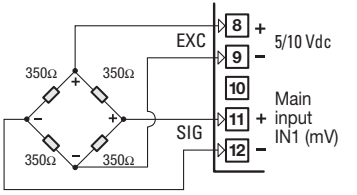


Configuration example:

- For strain gauge transducer rated 350Ω, 3.3 mV/V, 10 V excitation Voltage, select: I : 1, L : 2;


A3 6 wire Strain Gauge Input

- Set code L = 1 or 2 (see page 16) to obtain 5 or 10 Vdc stabilized power supply for the external strain gauge bridge, terminals 8 (+) and 9 (-).
- Set code I = 0, 1 or 2 (see page 16) to obtain suitable mV input (20, 50 or 100 mV), terminals 11 (+) and 12 (-).
- The calibration wires of the transducer must be connected to CAL terminals 34 and 35 (OP4 Output).

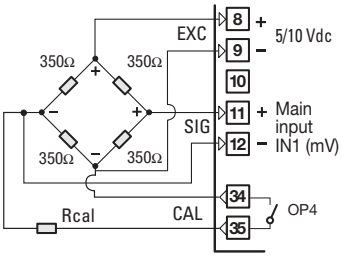


Note:
The excitation current of the strain gauge transducer must not exceed 30 mA.

B For mA, V




Rj >10MΩ.

B1 With 2 wire transmitter

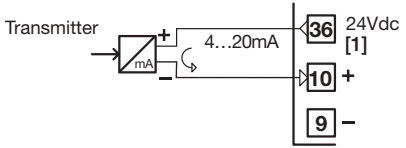

B2 With 3 wire transmitter

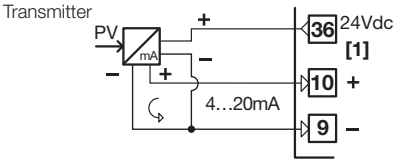


Note:

[1] Auxiliary power supply for external transmitter 24Vdc ±20% /30mA max. with no short circuit protection

2.3.3 AUXILIARY INPUT (IN2) (OPTION)


For mA and V

Current 0/4…20mA
Input resistance = 50Ω
Voltage:1…5V, 0…5V, 0…10V
Input resistence = 150kΩ



2.3.4 DIGITAL INPUTS

- The input is active when the logic state is ON, corresponding to the contact closed
- The input is inactive when the logic state is OFF, corresponding to the contact open

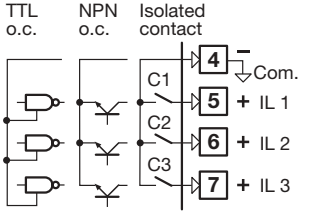

2.3.5 OP1 - OP2 (OPT.) - OP3 (OPT.) - OP4 OUTPUTS

OP1	SPDT relay output
OP2 - OP3	SPST-NO relay outputs
OP4	SPST-NO relay output
OP5	Retransmission analog output

OP1 relay output:

- SPDT relay,
  2A/250Vac for resistive loads;
  OP protection: use a 2AT at 250Vac fuse (for 4A/120Vac use a 4AT at 120Vac fuse).

OP2 - OP3 relay outputs

- SPST N.O. relay,
  2A/250Vac for resistive loads;
  OP protection: use a 2AT at 250Vac fuse (for 4A/120Vac use a 4AT at 120Vac fuse).

OP4 Relay output


- SPST relay N.O.,
  2A/250Vac for resistive loads;
  OP protection: use a 2AT at 250Vac fuse (for 4A/120Vac use a 4AT at 120Vac fuse).

OP5 isolated analog output


- 0/4…20mA, 750Ω/15V max..

2.3.6 ALARM OUTPUTS


OP1 output

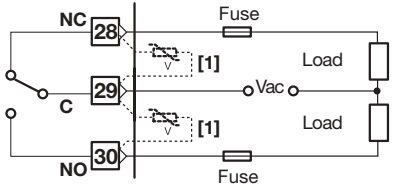

OP2, OP3 Outputs (opt.)

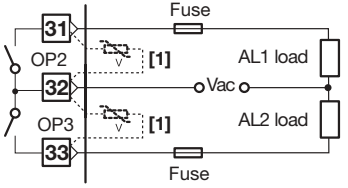


OP4 output

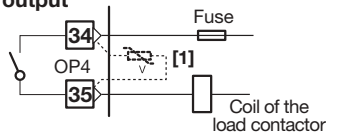

Notes:
[1] Varistor for inductive load 24Vac only;


2.3.7 OP5 ANALOG RETRANSMISSION OUTPUT (OPTION)




To retransmit one of the following values: IN1, IN2 or computed (conditioned) signal.

- Galvanic isolation 500Vac/1 min.
- 0/4…20mA, (750Ω or 15Vdc max.)

2.3.8 SERIAL COMMUNICATIONS (OPTION)



- Galvanic isolation 500Vac/1 min.
- Compliance to the EIA RS485 standard for Modbus/Jbus
- Setting dip switches

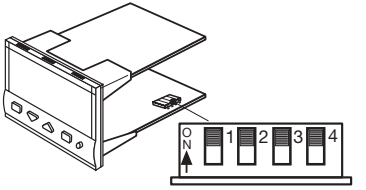


⚠ Please, read:
"gamma**due**® and delta**due**® series serial communication and configuration software" technical manual

3 PRODUCT CODING

The complete code is shown on the instrument label.

Information about product coding is accessible from the front panel by means of the procedure described in section 5.2 page 43.

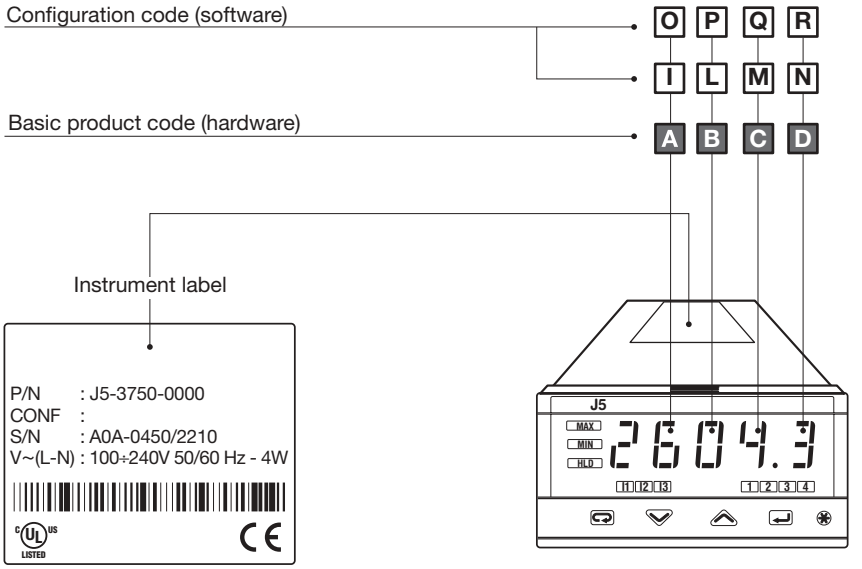

3.1 MODEL CODE

The product code indicates the specific hardware of the instrument.

	Line	Basic	Accessories	Configuration 1st part	Configuration 2nd part
Model:	J 5	A B C D	- 0 F 0 0	/ I L M N	- O P Q R

Line	**J 5**

Power supply	**A**
100...240Vac (-15...+10%)	**3**
24Vac (-25...+12%) or 24Vdc (-15....+25%)	**5**

Outputs OP1 - OP2 - OP3 - OP4	**B**
Relay / - / - / Relay	**7**
Relay - Relay - Relay - Relay	**9**


Serial Communications	**C**
None	**0**
RS485 Modbus/Jbus SLAVE	**5**

Options	**D**
None	**0**
Analog output for signal retransmission	**1**
Second input IN2	**2**
Analog output + Second input IN2	**5**


User manual	**F**
English (std)	**8**

3.2 CONFIGURATION CODING

A 4+4 index code follows the model of the indicator. The code has to be set to configure the indicator (see chapter 3.1 page 15)



E.g.: Enter the code 0020 to choose:
- Dc input 0...20 mV;
- Change the display color to red when AL1 is active;
- Peak hold disabled.



E.g.: Enter the code 2301 to choose:
- AL1 absolute, active high;
- AL2 absolute, active low;
- AL3 disabled;
- AL4 sensor break alarm.

IN1 Input range	IN1 Input Type	I	L
DC input 0... 20 mV	Linear	0	0
DC input 0... 50 mV		1	0
DC input 0... 100 mV		2	0
DC input 0... 1 V		3	0
DC input 0... 5 V		4	0
DC input 1... 5 V		5	0
DC input 0... 10 V		6	0
DC input 0... 20 mA		7	0
DC input 4... 20 mA		8	0
DC input 0... 20 mV	Strain gauge 5 V bridge excitation voltage	0	1
DC input 0... 50 mV		1	1
DC input 0... 100 mV		2	1
DC input 0... 20 mV	Strain gauge 10 V bridge excitation voltage	0	2
DC input 0... 50 mV		1	2
DC input 0... 100 mV		2	2

Notes:

1] Selecting for code **I** a value between 0... 3 the instrument uses, for the measurement, terminals 11 and 12. The other measurements (**I** values between 4... 8) are made using terminals 9 and 10.

2] To use a strain gauge input, select the bridge excitation voltage of the transducer. This selection is valid only if IN1 input range (code **I**) is set for mV input (codes 0... 2).

3] Selecting the strain gauge input enables the transducer excitation power supply, dedicated sensor break diagnostic routines (on terminals 8, 9, 11, 12) and a specific strain gauge menu. The bridge excitation voltage (5/10Vdc) is present on terminals 8, 9 when **L** = 1/2.


Display mode	M
Green	0
Red	1
Red when alarm 1 (AL1) active	2
Red when at least 1 alarm is active (alarm OR)	3
Alternate between IN1, IN2 and CIN value	4
Manual forced display of IN1, IN2, CIN, Lo, Hi and Unit value	5

Hold of the peak values	N
Disabled	0
Shows the max. value (HI peak) for a programmable period of time	1
Shows the min. value (LO peak) for a programmable period of time	2

Alarm type and function		O	P	Q	R
		AL1	AL2	AL3	AL4
Non-active		0			
Sensor or strain gauge break alarm		1			
Absolute	Active High	2			
	Active Low	3			
Deviation	Active High	4			
	Active Low	5			
Band	Active Out	6			
	Active In	7			
Rate alarm (AL1 only)		8	-		

4 OPERATIONS

4.1.1 KEY FUNCTIONS AND DISPLAY IN OPERATOR MODE

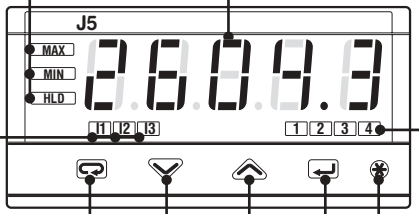

Display mode of the Peak values

MAX or MIN LEDs will be visible when the display shows a minimum or a maximum value. HLD LED will be visible when the value displayed is locked by the HOLD command. HOLD and PEAK commands stop the measurement procedure, while the PEAK VALUES HOLD command returns to normal operation after a programmed period of time (HLdEn parameter).

IN1 input value [1]

In engineering units

Over range

Under range

Digital input status LEDs (yellow)

I 1 - IL1 active
I 2 - IL2 active
I 3 - IL3 active

Alarm status LEDs (red)

1 AL1 ON
2 AL2 ON
3 AL3 ON
4 AL4 ON

Menu access

Alarm acknowledge

Min. and Max. values display

Entry key for selection and value confirmation

Note:

[1] The color of the display is set through field **M** of the Configuration Code (page 17).

4.1.2 KEY FUNCTIONS AND DISPLAY IN PROGRAMMING MODE

⚠


The parameter setting procedure has a timeout. If no keys are pressed for at least 30 seconds, the indicator automatically switches back to the operator mode. During the configuration procedure, the indicator does not exit the procedure for timeout.

After having selected the parameter or the code, press ⌃ or ⌄ to display or modify the value (see page 25).

The value is entered when the next parameter is selected, by pressing the ↵ key.

Until the ⌃ or ⌄ are pressed, or if you wait for 30 seconds, the parameter value is not enterted.

Pressing the ↻ key, the next group of parameters is shown on the display.

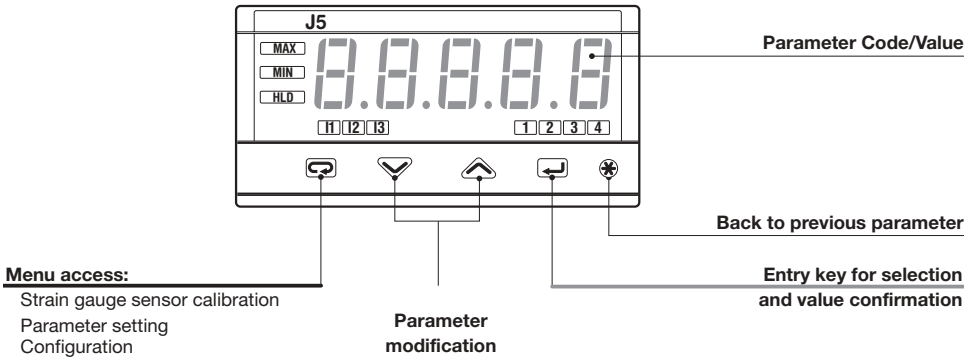


4.2 PARAMETER SETTING

4.2.1 NUMERIC ENTRY

(i.e. insert CodE3 password)


Pressing ∧ or ∨ momentarily changes the value by 1 unit every push.
Continued pressing of ∧ or ∨ changes first the unit value, then the value of the second digit, the third and so on.
If the value stops changing, the min./max. value has been reached.

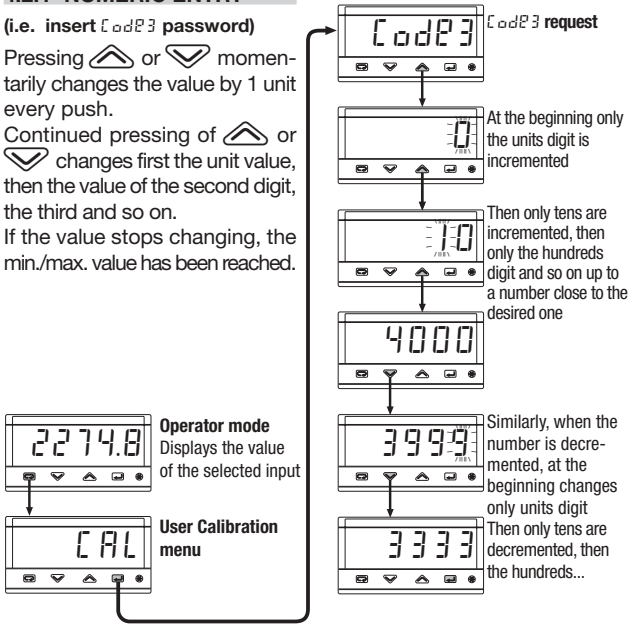

4.2.2 MNEMONIC CODES SETTING

(e.g. configuration see page 25)


Press the ∧ or ∨ to display the next or previous mnemonic for the selected parameter.
Continued pressing of ∧ or ∨ will display further mnemonics at a rate faster than one mnemonic every 0.5 s. The mnemonic displayed at the time the next parameter is selected is the one stored in the parameter.

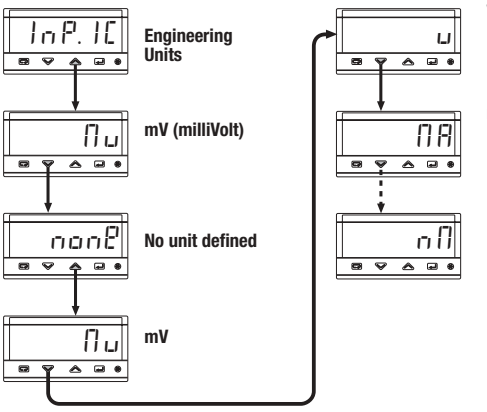

4.3 PARAMETERIZATION - MAIN MENU

This instrument has 3 levels of password protection which allow the administrator to protect access to the various menus.

Once the user selects the desired menu, the indicator prompts for the specific password. When all the passwords are set, `cod P1`, configuration (`conF`) can access all the menus, `cod P2`, the intermediate one (`Par`) can access the 2 less important menus (`cAL`, `Par`), `cod P3`, the third password allows the access only to the calibration menu (`cAL`).

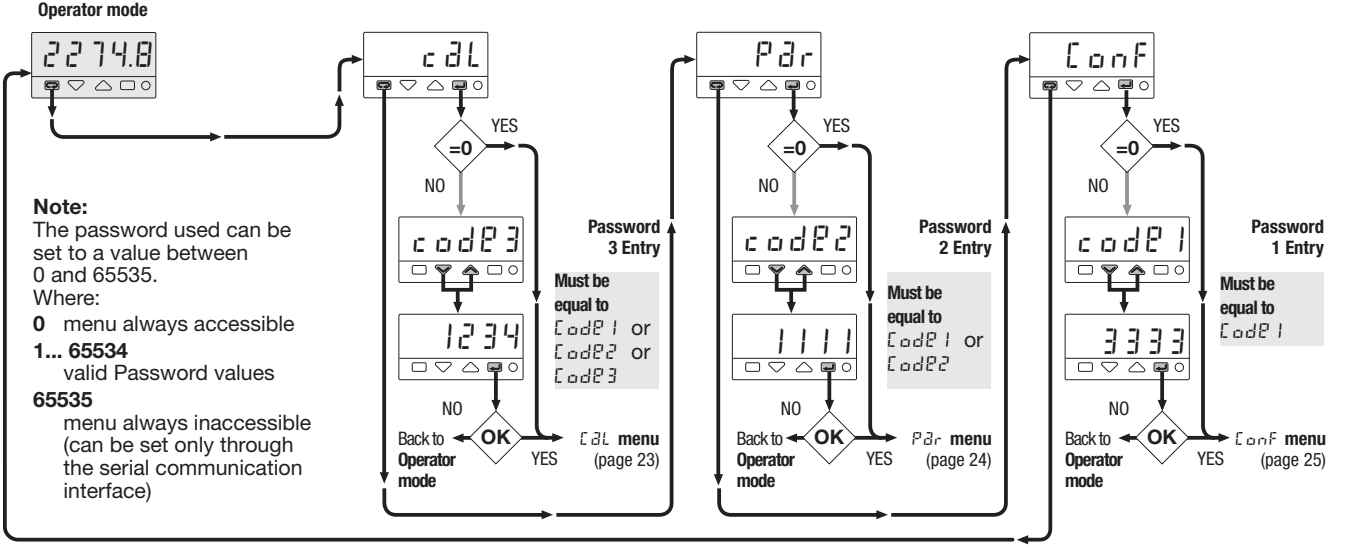

Note:
The password used can be set to a value between 0 and 65535.
Where:

0 menu always accessible

1... 65534
valid Password values

65535
menu always inaccessible (can be set only through the serial communication interface)

AVAILABLE PARAMETERS

CAL		User calibration menu
CodE 3		CAL menu password
tArE	Curr	Tare current value
	SEtt	Set tare
	CLEAr	Clear tare value
SCAL	2Eroc	Zero calibration
	hiCAL	Span calibration
EHit		Exit CAL menu

PAr		Parameter setting menu
CodE 2		PAr menu password
AL.SP	AL❑SP	Alarm Setpoint **[1]**
	AL.rEF	Alarm internal ref. value
AL.HAr	AL❑ hY	Alarm hysteresis **[1]**
	AL❑ d	Alarm activation delay **[1]**
MEAS	FiLtd	Filter time constant
	rESd	Display resolution
	HLdtM	Hold time
	dEF.Sh	Default display parameter
	t.MES	Alternate time
EHit		Exit PAr menu


Notes: [1] The parameter must be completed with the alarm number (❑ = 1... 4)

[2] The parameter must be completed with the output number (❑ = 1... 4)

ConF		Configuration menu
CodE 1		ConF menu password
bASE.C	Con.1	1st configuration code
	Con.2	2nd configuration code
	L. Fr9	Power supply frequency
InP.IC	Unit	IN1 engineering units
	in.Idd	Number of decimals
	tF iL1	IN1 filter constant time
	in.ILo	Low range
	in.IHi	High range
	in.ICn	Input conditioning
	Cut 1	Cut off square root
	in.ISh	Input shift
InP.2C	in.2St	IN2 input type
	in.2dd	Number of decimals
	tF iL2	IN2 filter constant time
	in.2Lo	Low range
	in.2Hi	High range
	in.2Cn	Input conditioning
	Cut 2	Cut off square root
	in.2Sh	Input shift
C inC	C in	Calculate value select
	C inLo	CIN Input Low Range
	C inHi	CIN Input High Range
	C indd	CIN no. of decimal

AoUt.C	AO.Src	Analog out Source
	AO.tYP	Analog Out Type
	AO.Lo	Analog Out Low Range
	AO.Hi	Analog Out High Range
AUX	iL 1	Digital Input1 Conf
	iL2	Digital Input2 Conf
	iL 3	Digital Input 3 Conf
	Prot	Communications protocol
	bAUd	Baud rate
	Par.Y	Parity
	Addr	Communications Address
	CodE 1	Password 1
	CodE2	Password 2
	CodE3	Password 3
ALM.C	AL❑Sr	Alarm Source **[1]**
	AL❑OP	Alarm Output **[1]**
	AL❑L b	Latching/blocking **[1]**
	ALM.Sr	Alarm Ref. Source
	OP.❑a	Output Action **[2]**
c.CAL	Sh.CAL	Shunt for strain gauge cal.
	CALMd	Calibration Mode
	SCCAL	Enable User cal. menu
	tArEM	Tare menu enable
	tArEE	Tare value editing enable
	FAct	Instrument calibration
EHit		Exit ConF menu

4.3.2 PARAMETERIZATION - CALIBRATION MENU

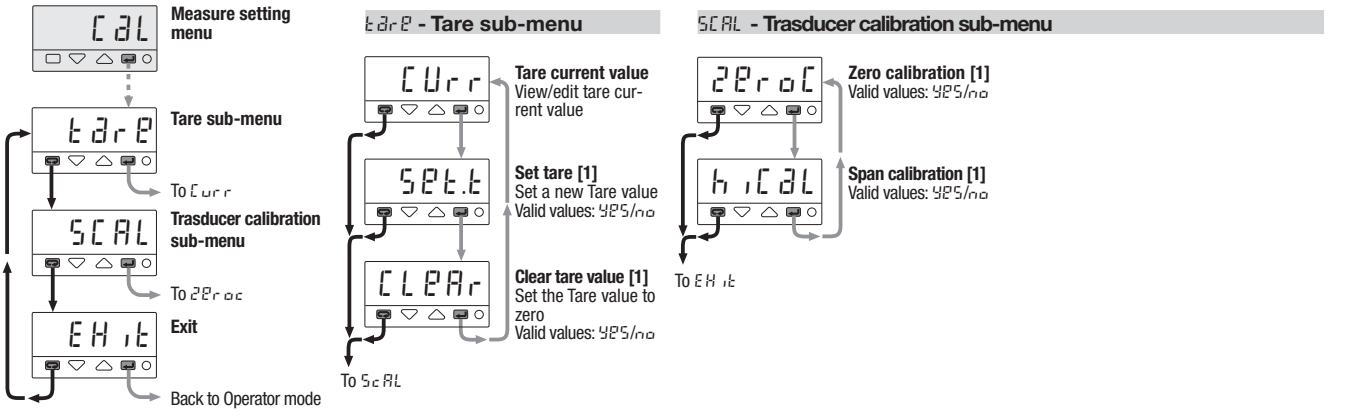


Note:

[1] When the user selects a command scrolling through the list with the ⟲ key, to accept the selected command, press the keys ⌃ or ⌄ to select:


YES the instrument executes the command as the user presses the ↵ key;

no the instrument switches to the subsequent command as the user presses the ↵ key


4.3.2 PARAMETERIZATION - PARAMETERS MENU

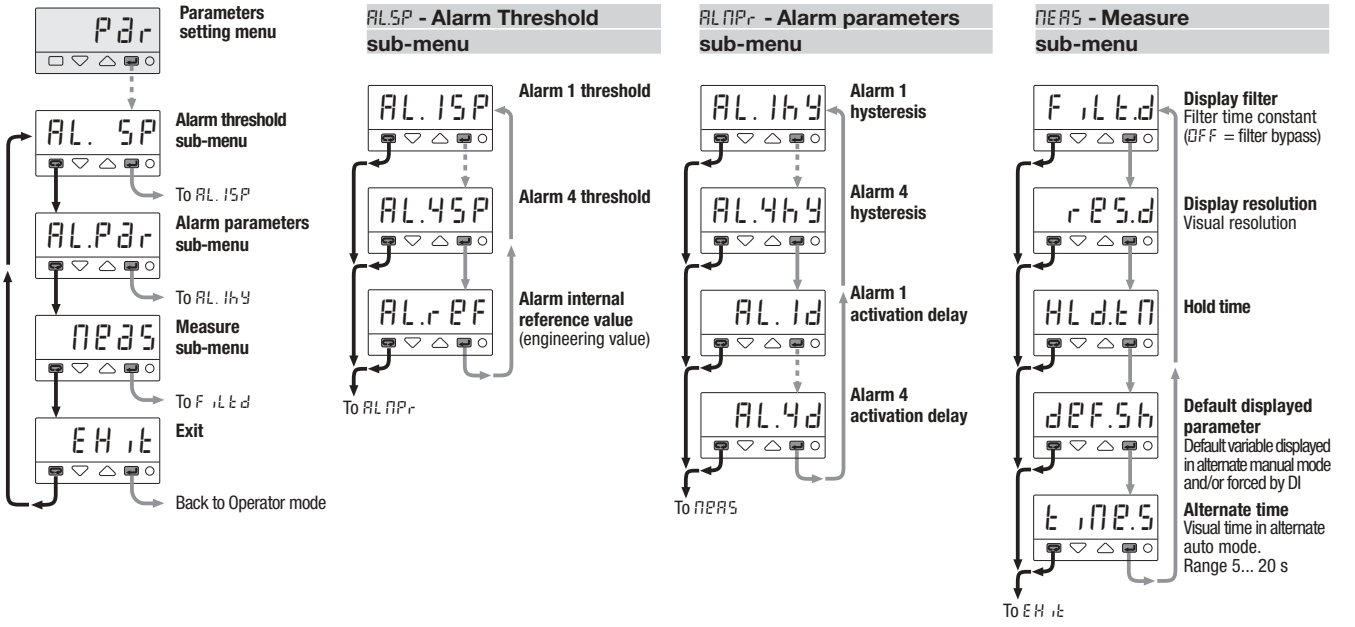


4.3.3 CONFIGURATION MENU

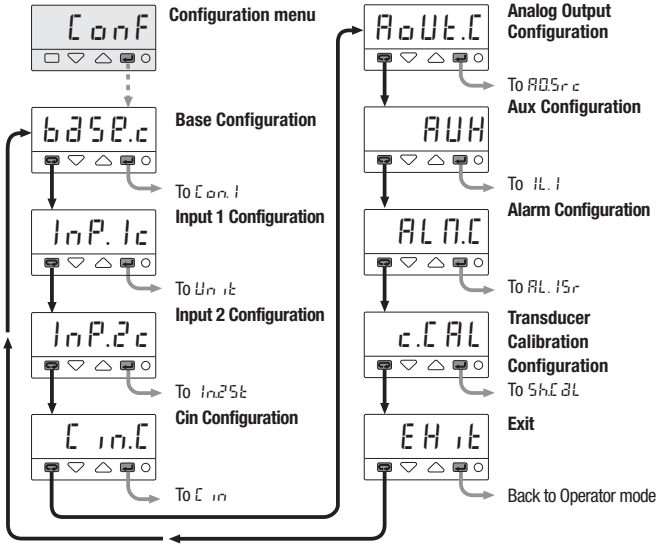


bASEC - Base Configuration sub-menu

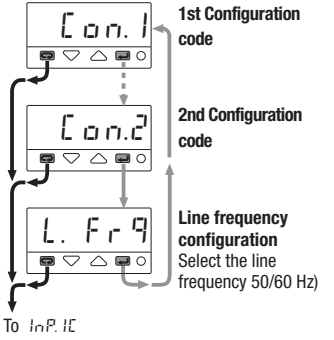

InP.1C - Input 1 Configuration sub-menu

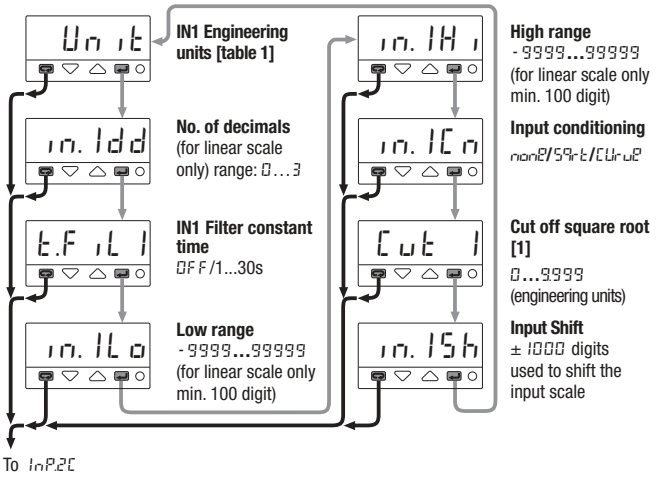

InP.2C - Input 2 Configuration sub-menu

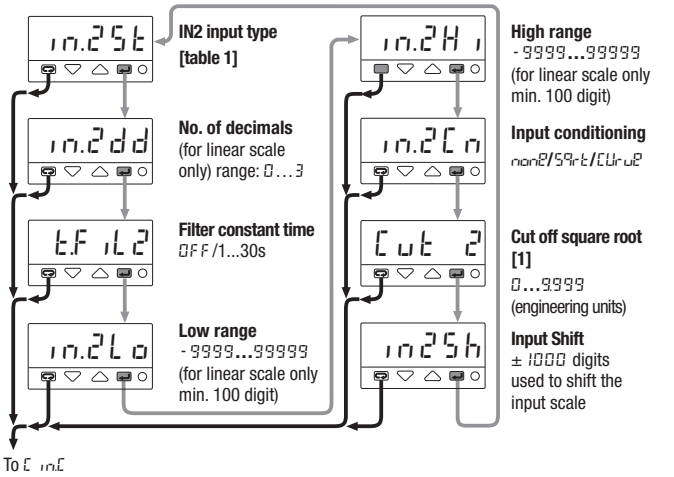


Note:

[1] Cut off the square root of the input value enables the user to round to zero a result that is too low to be important.


Table 1 - Engineering units

unit			
Value	Description	Value	Description
°C	Degrees Celsius	g	g (0.001 kg)
°F	Degrees Fahrenheit	kg	kg
none	none	ton	t (1000 kg)
mV	mV	q	q (100 kg)
U	Volt	hPa	hPa
mA	mA	MPa	MPa
A	Ampere	mbar	mbar
bar	Bar	mmH2O	mmH_2O
PSI	PSI	mmHg	mmHg
rh	Rh	kgm	kgm
PH	pH	Nm	Nm

CinC - CIN Configuration sub-menu

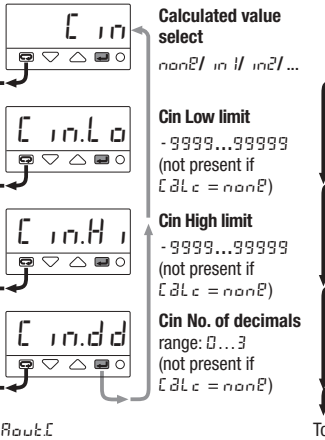

RoutC - Analog output Configuration sub-menu

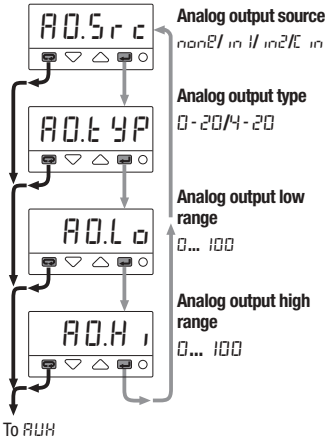

AUX - Auxiliary Parameters Configuration sub-menu


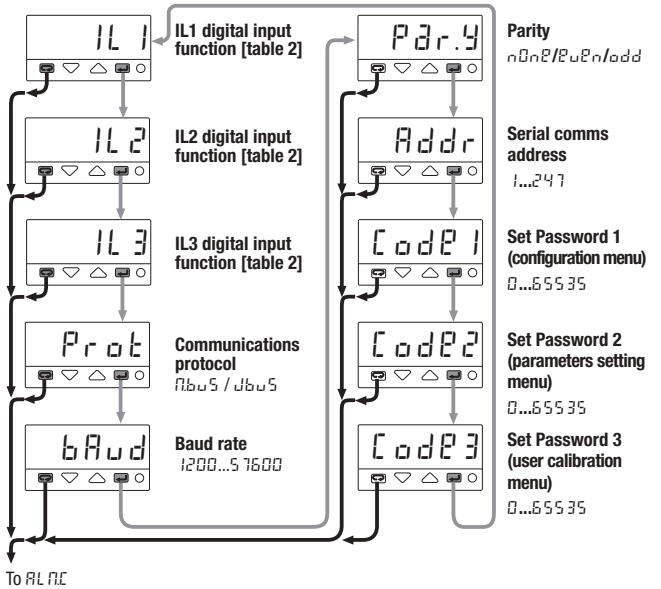



Table 2 - Digital input functions (see also page 38)

	IL 1	IL2	IL 3
Value	Description	Value	Description
nonE	Not used	HtPH	Positive peaks sustained display
tEY.1	Keypad lock		
OPbL	Outputs lock	HtPL	Negative peaks sustained display
AcE	Alarm acknowledge		
		F.d iS	Display a different parameter
r. HL	Max. and min. reset	SEtt	Set tare
		rESt	Reset tare
HoLd	Measure Hold	AC aL	Enable strain gauge calibration
HcPH	Positive peak enable	SC aL	Set calibration/Second calibration step (h iCaL)
HcPL	Negative peak (valley) enable		

AL.nE - Alarm configuration sub-menu

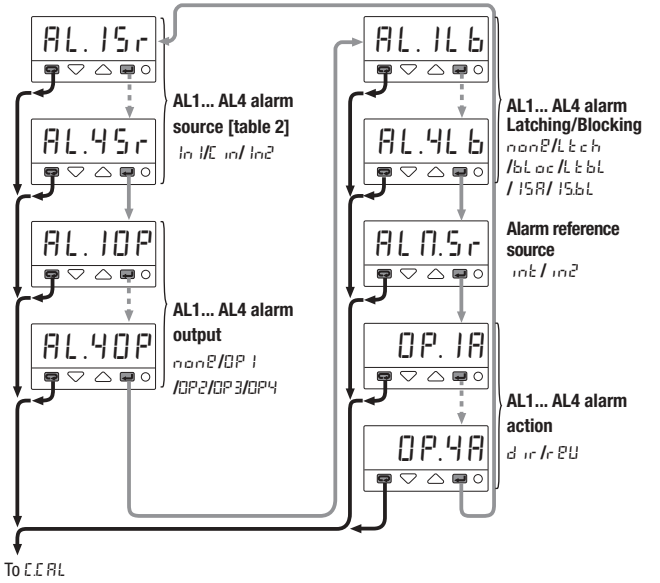

CCAL - Transducer Calibration sub-menu

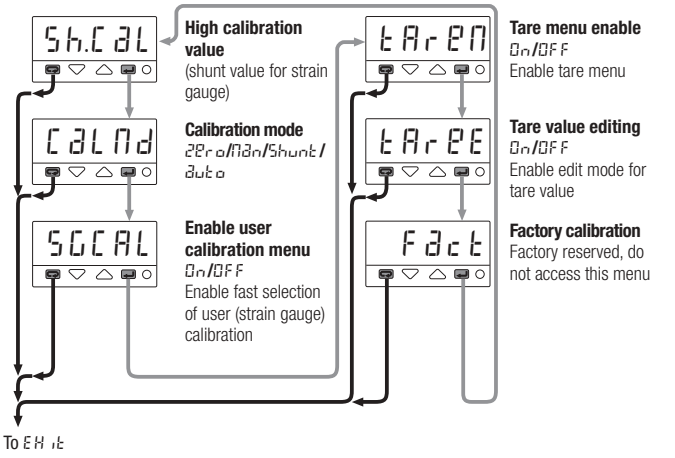

4.4 USER CALIBRATION MENU

To access the sensor calibration and the tare setting functions, the user must access the CAL menu and insert at least the 3rd level password (code 3 at page 39). If one of the passwords is set to zero, access to sensor calibration and tare setting functions is open.

tArE MENU

The tArE menu can be accessed only if the configuration parameter tArEN is set to On (page 42); in the tare menu are present the functions:

- Curr displays the current tare value or, if the configuration parameter tArE is set to On (page 42); it is possible to modify the tare value manually using the ∧ and ∨ (↵ enters the new value).
- SEtt sets a new tare value. Press the ∧ / ∨ keys to select the value YES (enable the tare setting), ↵ starts the setting process. During calibration, the instrument displays "run" and at the end "donE".
- CLEAr to reset the current tare value. Press the ∧ / ∨ keys to select the value YES, ↵ clears the tare value.

SCAL MENU

The SCAL menu can be accessed only if the configuration parameter SGCAL is set to On (page 42). Using the functions present in this menu, it is possible to calibrate the sensor on 2 different points: low range (2Proc) and high range (hicAL). The possible operations in this menu are determined by the configuration parameter cALd (page 42):

CALMd = Auto: 6 wire strain gauge automatic calibration

When the user sets and confirms the value On of the parameter 2Proc, the instrument starts the sensor calibration procedure (when the calibration starts, no load must be applied to the sensor). During this process, the instrument calculates and stores the offset from zero, then inserts the shunt resistance (closing OP4 relay), changes the measured value to the hicAL configuration parameter, calculates the span value, stores the calculated value and returns to the normal operation mode.

CALMd = Shunt: 6 wire strain gauge calibration

This procedure is similar to the previous one except for the fact that, once calibrated at zero, to start the calibration process of the second point the user must select and confirm the value On for the hicAL parameter.

CALMd = Man: manual calibration

The operation is similar to the calibration with the shunt, but when activated, the calibration of the second point does not activate OP4 (can be used for different purposes, e.g. as alarm). The two points can be calibrated separately and independently.

CALMd = 2Pro: single calibration

This setting allows only the zero calibration procedure (in the menu is present only the parameter 2Proc).

4.4.1 CALIBRATION AND TARE PROCESS

The process that calculates the tare value or the calibration of the strain gauge, performs several functions in order to make the reading more accurate.
If the functions to not pass, the instrument displays an error code that indicates the problem found.
To correctly understand the meaning of the error messages, some aspects of the calibration or the tare setting processes must first be explained.

- For both the processes, the input must be acquired in a known and stable condition to avoid that electrical noise, mechanical disturbances or variations of the input signal can change the quality of the reading. The instrument uses an algorithm that verifies the stability of the input signal and returns an error if it is not stable.
- The strain gauge calibration process defines the zero and a measurement span. On these two measurements a control can be made to avoid that a too small of a span value does not result in a resolution better than or equal to 10 bits.
- Further control is made on the strain gauge calibration in order to verify that the instrument is able to measure the whole range as the calibration process of the high end is made at a value that is 50... 100% of the full range.

Error messages:

Code	Description	Solution
Err2	Tare not set because the input signal is not stable	Check the cable wiring. Check for noise sources.
Err3	Strain gauge sensor not correctly connected	
Err4	Low range calibration command not executed because the input signal is not stable	
Err5	High range calibration command not executed because the input signal is not stable	
Err6	Strain gauge calibration span lower than 10 bit resolution	Change the input range
Err7	The instrument does not cover the whole strain gauge measure range	
Err8	Low range of strain gauge calibration out of range	

4.5 PARAMETER DESCRIPTION

For ease of operation of the indicator, parameters have been grouped (menu) according to their functional area.

4.5.1 ALARM THRESHOLD SUB-MENU

OP1, OP2, OP3 and OP4 outputs can be used as alarms.
It is possible to configure up to 4 alarms: AL1, AL2, AL3 and AL4 (page 24)selecting for each of them:

- type and operating condition of the alarm (page 34);
- functionality of the alarm acknowledgement (latching) Ltch (page 40);
- start up disabling (blocking) bLoc (page 40);
- Sensor or strain gauge break function (page 34);
- Rate alarm (only for AL1 referred to IN1) (page 34).

AL.1SP **AL1 alarm threshold**
AL.2SP **AL2 alarm threshold**
AL.3SP **AL3 alarm threshold**
AL.4SP **AL4 alarm threshold**

Parameters to set the threshold of AL1, AL2, AL3 and AL4 alarms.

The range of the alarm threshold corresponds to the whole span.

When an alarm occurs, the display will show the red LEDs 1, 2, 3 and 4 respectively ON and, when configured, with a change of the display color, if configured.

AL.rEF **Alarms reference value**

Internal reference value for deviation and band alarm. Used when AL.Sr = int (page 41).

4.5.2 ALARM PARAMETER SUB-MENU

AL.1hy **AL1 alarm hysteresis**
AL.2hy **AL2 alarm hysteresis**
AL.3hy **AL3 alarm hysteresis**
AL.4hy **AL4 alarm hysteresis**

Hysteresis of the threshold of AL1, AL2, AL3 and AL4 alarms. It is specified as a % of the full range.

AL.1d **AL1 alarm activation delay**
AL.2d **AL2 alarm activation delay**
AL.3d **AL3 alarm activation delay**
AL.4d **AL4 alarm activation delay**

Specifies a time (in seconds) that the indicator waits before activating an alarm. Range 0.0...60s in steps of 0.1 s.

4.5.3 MEASURE MANAGEMENT SUB-MENU

The entries present in the menu allow the user to configure:
- Display filter;
- Measure peak hold time;
- Display resolution;
- The default display parameter;
- Alternate display period.

Display filter

This parameter configures the period of time a redout must be sustained before diplayed.
Setting range: 1...30.0 s.
Default value: OFF (filter bypass).

Measure peak hold time

This parameter allows the configuration of a period of time the peak value will be maintained on the display.
Setting range: 0.5...999.9 s.

Display resolution

This parameter defines the resolution (in digits) that the instrument applies to the display output to make the readout more stable.
Setting range: 1/5/10/20/50/100.
Default value: 5.

Default displayed variable

Defines the name of the variable that is displayed by default when in manual forced display mode (field **M** set to 5) in the configuration code.

Value	Description
In1	Input 1
In2	Input 2
Cin	Conditioned input

Default value: In1

Alternate display period (Cin active)

Parameter to set the display time of an alternate measure when the conditioned input is active (Cin).
Setting range: 5...60 s.
Default value: 5 s.

4.6 CONFIGURATION MENU

For ease of operation of the indicator, all parameters have been organized in groups (menu), according to their functional area.

4.6.1 BASE CONFIGURATION SUB-MENU



1st part of the configuration code

Field **I** allows the selection of the range of the primary input (IN1 page 17); code **L** allows the selection the strain gauge input.

Field **M** allows the selection of the function mode of the display (page 17).

Field **N** selects if and how the peak values are to be held (or not) on the display.



2nd part of the configuration code


Fields **O** **P** **Q** and **R** select alarm type and function (page 17).

SENSOR OR STRAIN GAUGE BREAK ALARM FUNCTION

During the configuration phase (page 17) set fields **O** , **P** , **Q** , **R** , to value 1. When the PV overcomes the sensor range limits, the sensor break alarm intervention is immediate. **When the alarm condition is no longer present, the alarm stops.**


ABSOLUTE ALARM

During the configuration phase (page 17) set fields **O** , **P** , **Q** , **R** , to value 2 (actve high) or 3 (active low).

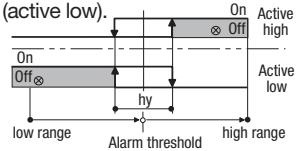


DEVIATION ALARM

During the configuration phase (page 17) set fields **O** , **P** , **Q** , **R** , to value 4 (active high) or 5 (active low).



BAND ALARM

During the configuration phase (page 17) set fields **O** , **P** , **Q** , **R** , to value 6 (active in) or 7 (active out).




AL1 RATE ALARM FUNCTION

During the configuration phase (page 17) set field **O** , to value 8. When the changing rate of the PV connected to the alarm is higher than the specified threshold, AL1 is activated.

Setting range: 0.1... 5.0 digit/s.

For rates between 0.1... 1.0 digit/s, AL1 will be activated after 6...1 s. For rates between 1...5 digit/s, AL1 will be activated after 1s...40ms.



Line configuration frequency

In order to optimize the rejection to line frequency it is necessary to set this parameter to the correct value (50/60 Hz).

4.6.2 IN1 CONFIGURATION SUB-MENU

Engineering units

This parameter sets the desired engineering units. All the engineering units available are listed on page 27, table 1.

IN1 Input number of decimals

This parameter allows the user to set the number of decimals to be displayed for the primary (IN1) input.


For linear scales only.

Setting range: 0...3

IN1 **Input 1 filter time constant**

Time constant, in seconds, of the RC input filter applied to the PV input.

When this parameter is set to 0 the filter is bypassed.

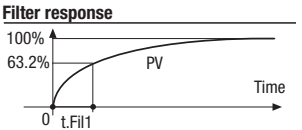

Setting range: 0...30.0 s.

IN1 input low range

IN1 input high range

These parameters allow the user to set the operating range of the primary (IN1) input. For linear scales only.

Setting range: -9999...99999

IN1 measure conditioning

Parameter to enable the conditioning of the IN1 measure. The calculations available are: square root of IN1 measure (Sqrt);

16 segments (or 17 points) linearisation (CUrvE).

When the value is nonE, no calculation is made on the IN1 measure.

⚠ The 17 points to define the linearisation curve must be entered through the serial communications port; please, read: the "gamma**due**® and delta**due**® series serial communication and configuration software" technical manual for more information.

Cut-off square root result

This parameter allows the user to round to zero those results of the square root of IN1 conditioning that are not meaningful (Sqrt).

Setting range: 0...9999.

Default value: 0.

IN1 input shift

This value is added to the measured IN1 value. Its effect is to shift the whole IN1 scale of up to ±1000 digits.

Default value: 0.

4.6.3 IN2 CONFIGURATION SUB-MENU

IN2 input type

The parameter defines the range of the secondary input (IN2).

Value	Description
0-5	0...5 V
1-5	1...5 V
0-10	0...10 V
0-20	0...20 mA
4-20	4...20 mA

Number of decimals IN2 input

This parameter allows the user to set the number of decimals to be displayed for the secondary input (IN2).


For linear scales only.

Setting range: 0...3

Input 2 filter time constant

Time constant, in seconds, of the RC input filter applied to the PV input.

When this parameter is set to 0 the filter is bypassed.

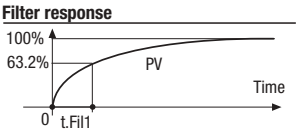

Setting range: 0...30.0 s.

IN2 input low range

IN2 input high range

These parameters allow the user to set the operating range of the primary (IN2) input. For linear scales only.

Setting range: -9999...99999

IN2 measure square root

Parameter to enable the calculation of the square root of IN2 measure (Sqrt = enabled, nonE = disabled).

Cut-off square root result

This parameter allows the user to round to zero those results of the square root of IN2 conditioning that are not meaningful

Setting range: 0...9999.

Default value: 0.

Secondary input (IN2) shift

This value is added to the measured input 2 value. Its effect is to shift the whole IN2 scale of up to ±1000 digits.

Default value: 0.

4.6.4 CONDITIONED INPUT CONFIGURATION SUB-MENU

Calculated value selection (Cin)

The Cin parameter selects the type of operation that must be applied to input 1 (IN1) using the secondary input (IN2); the result is the conditioned input (C in).
In the table that follows are listed the possible conditioning operations:

Id	Description
in1	Cin = IN1
in2	Cin = IN2
SuM	Cin = IN1 + IN2
Sub	Cin = IN1 - IN2
Avg	Cin = (IN1 + IN2)/2
HIG	Cin = MAX (IN1, IN2)
LoW	Cin = Min (IN1, IN2)
MUL	Cin = IN1 * IN2
rtio	Cin = IN1/IN2

Low range for conditioned value

High range for conditioned value

These parameters define the range for the conditioned measure (C in).

Number of decimals for Cin value

This parameter allows the user to set the number of decimal digits to be displayed for the primary (IN1) input.

Setting range: 0...3

4.6.5 ANALOG OUTPUT CONFIGURATION SUB-MENU

Analog output source

Selects the variable to be put on the analog output.

Setting values: None, In1, Cin, In2.

Analog output type

Selects the type of signal retransmitted by the analog output.

Values: 0... 20 mA, 4... 20 mA.

Default value: 0...20mA.

Analog output low range

Analog output high range

Range of the analog output:

AoLo: -9999...99999

AoHY: -9999...99999

Default values:

AoLo: 0

AoHY: 10000

4.6.6 AUXILIARY PARAMETER CONFIGURATION SUB-MENU

IL1 digital input function

IL2 digital input function

IL3 digital input function

A function is assigned through the configuration procedure to each IL1, IL2 and IL3 digital input (see the parameters setting at table 2 at page 28).
The configured function is activated when the digital input (free voltage contact or open collector output) is in the ON state (closed). It is deactivated by setting the input to the OFF state (open).
The activation of the function through the digital input has the highest priority than through the keypad or through the serial communications.

Function	Parameter Value	Performed operation		Notes
		Off	On	
None	nonE	—	—	Not used
Keypad lock	tEY.1	Unlocked	Locked	With the keypad locked the commands from digital inputs and serial communications are still operating
Outputs lock	OP.bL	Normal operation	Outputs lock	Closing the contact causes the setting to the logical status 0 of the output ports. The retransmission analog output is forced to the low limit (0 or 4 mA)
Alarm acknowledge	AcK	Normal operation	Alarm acknowledge	Closing the contact causes the acknowledgement of the active alarms
Peak and Valley value reset	r. HL	Normal operation	Reset Peak and Valley	Closing the contact causes the reset of the stored maximum and minimum value
Measure hold	HoLd	Normal operation	Measure hold locked	Closing the contact locks the measurement of the IN1 input. In accordance, all the values directly connected to IN1 measure are locked.
Positive peak hold enable (peak)	HcPH	Normal operation	Shows the max. value read	The display shows the maximum value read all the time the contact is closed. The number displayed changes in case of higher max. values
Negative peak hold enable (valley)	HcPL	Normal operation	Shows the min. value read	The display shows the minimum value read all the time the contact is closed. The number displayed changes in case of lower min. values
Positive peaks sustained display	HtPH	Normal operation	Max. value + normal operation	The display shows, for a programmable period of time (HL dt), the max. value read, then returns to normal operation
Negative peaks sustained display	HtPL	Normal operation	Min. value + normal operation	The display shows, for a programmable period of time (HL dt), the min. value read, then returns to normal operation
Display a different parameter	Fd,S	Normal operation	Alternate display	For all the period the contact is closed the display shows the value of the variable set with the dSPSh parameter
Set Tare	SEt.t	Normal operation	Set the new tare value	Closing the contact causes the storing of the PV as tare value
Reset Tare	rESt	Normal operation	Reset the tare value	Closing the contact causes the reset of the stored tare value
Enable automatic calibration	a.cAL	Normal operation	Enable calibration	Closing the contact enable the automatic calibration process of the strain gauge (see page 30)
Start automatic calibration	S.cAL	Normal operation	Start calibration	Closing the contact causes the starting of the automatic strain gauge calibration

SERIAL COMMUNICATION PARAMETERS (OPTIONAL)

The parameters that follow are displayed only when the optional RS485 serial communications is installed in the instrument.

Communications protocol

Baud rate

Parity

Instrument serial address

Setting values:
Protocol: Modbus/Jbus.
Baud rate: 200/2400/4800/9600/19200/38400/57600 baud.
Parity: nonE/EuEn/odd.
Instrument serial address: 1...247
Default values:
Protocol: Jbus.
Baud rate: 9600 baud.
Instrument serial address: 1
Parity: nonE.

SAFETY PARAMETERS

Set Cal menu access code (1)

Set Par menu access code (2)

Set Conf menu access code (3)

These parameters allow the user to change the factory default passwords.
When one code is set to zero , access to the menu(s) connected to that code is (are) accessible (see page 21). When, using the serial communications port, and the user sets a code to 65535, the menu(s) connected to that code is (are) locked.
Setting ranges: 0...65534 (the value 65535 can be set only from the serial communications port)
Default values:
Code1: 3333
Code2: 1111
Code3: 1234

4.6.7 ALARM PARAMETERS CONFIGURATION SUB-MENU

The entries of this menu allow the user to configure the functioning parameters of alarms AL1, AL2, AL3 and AL4.

AL1 alarm source

AL2 alarm source

AL3 alarm source

AL4 alarm source

Sets, for each alarm, the signal source to be considered.
Setting values: IN1, Cin; IN2.
Default value: IN1

AL1 alarm output

AL2 alarm output

AL3 alarm output

AL4 alarm output

These parameters connect each alarm to the output port to be activated when an alarm condition occurs.
Setting values:
none, OP1, OP2, OP3, OP4
Default values: **AL1:** OP1
AL2: OP2,
AL3: none
AL4: none.

AL.1Lb
AL.2Lb
AL.3Lb
AL.4Lb

AL1, AL2, AL3, AL4 latching and blocking function

For each alarm, it is possible to select one of the following functions:


- none; none
- Ltch acknowledge;
- bLoc blocking;
- Lt.bL latching + blocking
- ISA ISA ack. sequence
- IS.bL ISA ack. sequence + blocking

Ltch ALARM ACKNOWLEDGE FUNCTION


Once an alarm occurs it is indicated on the display until it is acknowledged. To acknowledge an alarm press the ⊛ key. **After this operation, the alarm changes state only when the alarm condition is no longer present.**

bLoc START-UP DISABLING

Ramp down



Ramp up



ΔAL Threshold = REF ± range

ISA "ISA A" ALARM RESET SEQUENCE

The alarm intervention activates both the visual alarm (the alarm LED on the display) and the audible alarm (the OP output used to activate for example a buzzer or a siren). When the operator acknowledges the alarm, the status of the two alarms differ if the alarm condition has been removed or not. In the table that follows, the visual and audible alarm status are pointed out for each condition.

Status	Status changes				Visual alarm (alarm LED)	Audible alarm (OP output)
	Input variable		Reset (ACK)			
	Normal condition	Alarm condition	Reset not done	Reset done		
No alarm active	No status changes	Go to status: **Alarm not acknowledged**			OFF	OFF
Alarm not acknowledged			No status changes	Go to status: **Acknowledged alarm**	Flashing	Active
Acknowledged alarm	Go to status: **No alarm active**	No status changes			Steady ON	OFF

Alarm reference source

This parameter allows the user to select the reference value to be used for the alarms.

Values: Int/In2/Cin

Default: Int (the value set in ALrEF page 32).

Output OP1 action

Output OP2 action

Output OP3 action

Output OP4 action

Sets the type of action of the output port.

Values: direct (relay-coil activated in alarm condition), **reverse** (relay-coil not activated when in alarm condition).

Default value: direct.

4.6.8 TRANSDUCER CALIBRATION SUB-MENU

The CAL menu allows the user to choose the transducer calibration mode.

Shunt for strain gauge calibration

This parameter sets the value, in percentage, of the higher calibration point of the strain gauge (the shunt value).

Setting range: 50...100%

Default: value: 80% (standard value of the 6 wire strain gauge shunt).

Transducer calibration mode

This entry selects the type of calibration procedure to be performed.

Setting values: 2Pro, Man, Shunt, Auto

2Pro	Enables only the zero calibration
Man	Both the Zero and Span are enabled. The calibration processes are started through separate operator commands. OP4 output is not associated to the span calibration phase.
Shunt	Both the Zero and Span are enabled. The calibration processes are started through separate operator commands. OP4 relay is associated to the Span calibration phase and is activated automatically in order to insert the shunt of the 6 wire strain gauge.
Auto	Both the Zero and Span are enabled. The calibration processes are started through an operator command. OP4 relay is activated automatically in order to insert the shunt of the 6 wire strain gauge.

Enable sensor calibration

Enable set tare command

Enable/Disable access to the transducer calibration sub-menu (page 23) and to tArP sub-menu (page 23). When both are disabled, the SCAL menu is hidden.

Setting values: ON/OFF

Default value: ON.

Enable edit tare

Enable/Disable the editing of the tare value with the Curr command (page 30).

Setting values: ON/OFF


Default value: ON.

Factory calibration


⚠ The instrument calibration is a factory procedure. It can be performed by the end user with caution. The menu is protected with a password.

5 DISPLAYS

5.1 DISPLAYING THE PROCESS VARIABLES [1]

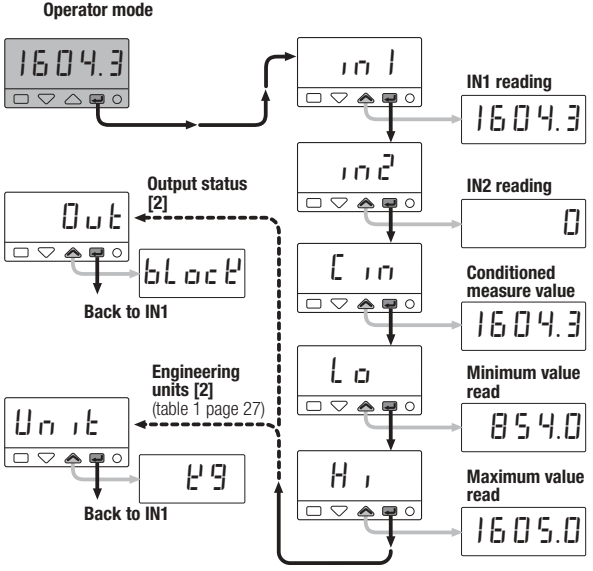

5.2 DISPLAYING THE CONFIGURATION CODES [1]

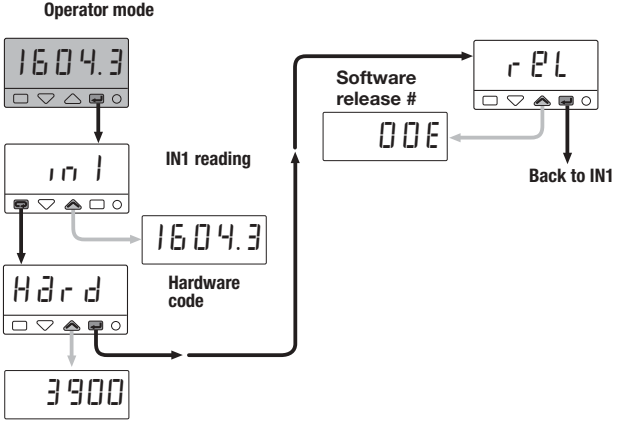

Notes:

[1] To exit the Display functions and return to the Operator mode, wait 5 seconds without touching the instrument buttons.

[2] bLocK is displayed when the outputg are locked (page 45), Unit is displayed when the outputs are unlocked.

6 COMMANDS

COMMANDS TO THE INDICATOR AND OPERATING PROCEDURE

The commands can be entered in 3 ways:




6.1 KEYPAD

see page 45

- Keypad lock
- Outputs lock

6.2 DIGITAL INPUTS

see page 32



6.3 SERIAL COMMUNICATIONS

see the manual on this topic



6.1 KEYPAD COMMANDS


6.1.1 KEYPAD LOCK/UNLOCK

To lock/unlock the keypad, press and hold the keys [↩] and [↵] simultaneously for 2 seconds. With keypad locked, if the user presses a key, the instrument displays the message "Loct".

The keypad lock/unlock can also be achieved over serial communications.

⚠ The keypad lock is retained in the event of power failure.

Operator mode

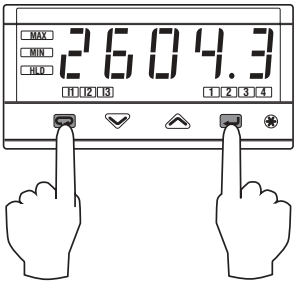

Press simultaneously for 2 seconds


6.1.2 OUTPUT LOCK/UNLOCK

The outputs are switched to the OFF status by pressing and holding the keys [↩] and [▽] simultaneously for 2 seconds. With the outputs locked, when displaying the process variables the instrument displays the message "bLoCk" instead of "Unit".
To unlock the outputs press the keys simultaneously again.

The outputs lock/unlock can also be achieved over serial communications.

⚠ The outputs lock is retained in the event of power failure.

Operator mode

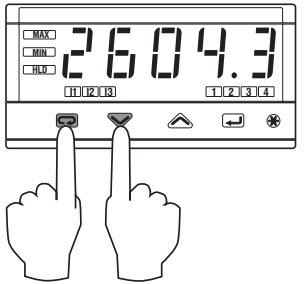

Press simultaneously for 2 seconds

7 TECHNICAL SPECIFICATIONS

Features (at 25°C env. temperature)	Description			
Dual color display	5 digit, high efficiency, height 15 mm, limits: -9999...99999 red or green configurable depending on the user needs and/or the alarm status			
IN1 Main input (see pages 11,12 and 16)	Common characteristics	A/D converter with 16 bit resolution Overall response time: 20 ms Input shift: ±1000 digit Input filter: 1...30 s (OFF= 0)		
	Accuracy	0.1% ±1 digit; between 85...240 Vac the error is negligible		
	Strain gauge bridge excitation	5V/10V selectable	350Ω...10kΩ bridge load	
	DC input Current	0/4...20 mA	Engineering units, Floating decimal point, Display resolution: 1, 2, 5, 10, 50, 100 digits selectable	Accuracy 0.1% Sampling rate 20 ms Input drift: <0.1%/20°C ambient temperature
	DC input Voltage	0...20 mV 0...1 V 0...50 mV 0...5 V 0...100 mV 0...10 V		
IN2 second input (option)	DC Current	0/4... 20 mA R input = 60Ω	Accuracy 0.1% Sampling rate 250 ms	
	DC Voltage	1/0...5, 0...10 V		
Digital inputs (3 logic not isolated from internal electronics)	The voltage free contact closure enables:	Keyboard lock, Output block, Alarm acknowledge, Min./Max. reset, Measure hold, Peak or Valley hold, Display variable select, Strain gauge calibration, Tare set		

Features (at 25°C env. temperature)	Description				
OP1 output	SPDT relay, 2A/250Vac (4A/120Vac) for resistive load				
OP2 output (opt.)	SPST relay N.O., 2A/250Vac (4A/120Vac) for resistive load				
OP3 output (opt.)	SPST relay N.O., 2A/250Vac (4A/120Vac) for resistive load				
OP4 output	SPST relay N.O., 2A/250Vac (4A/120Vac) for resistive load				
OP5 analog output (option)	0/4…20mA, 750Ω/15V max. To retransmit: IN1, IN2 or CIN Accuracy: 0.1% Resolution: 12 bit Galvanic isolation: 500Vac/1min				
AL1 - AL2 - AL3 - AL4	Hysteresis	0.1…10.0%			
	Action	Active high	Action type	Changing rate threshold	0.1...5.0 digit/s
				Deviation threshold	± range
		Active low		Band threshold	0…range
				Absolute threshold	whole range
		Special functions	Strain gauge break, Sensor break, Acknowledge (latching), Activation inhibit (blocking), OR'ed of different sources of alarms, ISA-A acknowledge sequence for activation of visual and audible alarm		

Features (at 25°C env. temperature)	Description		
Serial comms. (optional)	RS485 isolated, Modbus/Jbus protocol, 1200, 2400, 4800, 9600, 19200, 36400, 56800 bit/s, 3 wire		
Auxiliary power supply	+24Vdc ±20%, 30 mA max. for a 4... 20 mA, 2 wire transmitter		
Operational safety	Input measure	Detection of out of range, short circuit or sensor break with automatic activation of the safety strategy and alerts on display	
	Parameters	A non volatile memory stores for unlimited time all the configuration and parameter values	
	Access protection	3 password levels to access the strain gauge calibration, Configuration and Parameters data, Keyboard lock, Outputs Block	
General characteristics	Power supply	100...240Vac (-15...+10%) 50/60Hz or 24Vac (-25...+12%) 50/60Hz and 24Vdc (-15...+25%)	Power consumption 4W max. (PTC protected)
	Safety	Compliance EN61010-1 (IEC 1010-1), installation class 2 (2.5kV) pollution class 2, class II instrument	
	Electromagnetic compatibility	Compliance to the CE standards for industrial systems and equipment	
	UL & cUL approval	File E176452 (pending)	
	Protection EN60529 (IEC529)	IP65 front panel	
	Dimensions	1/8 DIN - 96 x 48, depth 110 mm, weight 250g approx.	

WARRANTY

We warrant that the products will be free from defects in material and workmanship for 3 years from the date of delivery.
The warranty above shall not apply for any failure caused by the use of the product other than as instructed in this manual.

■ ICON TABLE

Main universal input	
SG	Strain gauge input
Custom	Custom
LIN	Linearize Custom input
mA V	mA and mV
TC	Thermocouple
Pt100	RTD (Pt100)
Hz	Frequency
ΔT	Delta Temp (2x RTD)

Special Functions	
MIN	Display the minimum stored value
MAX	Display the maximum stored value
HOLD PEAK	Hold peaks or valleys
HOLD PV	Hold the PV
CIN	Conditioned Input
NO/NC	NO/NC Alarm status
	Keypad lock
	Outputs lock

Auxiliary input	
	Current transformer
REM mA	mA Remote setpoint
REM V	Volt Remote setpoint
POT.	Feedback potentiometer

Digital input	
	Isolated contact
	NPN open collector
	TTL open collector

Setpoint	
LOC	Local
STAND BY	Stand-by
START UP	Start-up function
TIMER	Timer function
MEM	Memorized
REM	Remote
	Setpoint programmer

Digital input connected functions	
	Auto/Manual
RUN	Run, Hold, Reset and program selection
HOLD PV	PV hold
SP SLOPE	Setpoint slopes inhibition

Output	
	SPST Relay
	Triac
	SPDT Relay
mA	mA
mA V	mA mV
	Logic

ASCON WORLDWIDE SALES NETWORKS

SUBSIDIARY

FRANCE

ASCON France

2 bis, Rue Paul Henri Spaak
ST. THIBAULT DES VIGNES
F-77462 LAGNY SUR MARNE - Cedex
Tél. +33 (0) 1 64 30 62 62
Fax +33 (0) 1 64 30 84 98
ascon.france@ascon.fr

Agence Sud-Est

Tél. +33 (0) 4 74 27 82 81
Fax +33 (0) 4 74 27 81 71

USA

ASCON Corporation

1884 East Fabyan Parkway
Batavia, Illinois 60510
Tel. +1 630 482 2950
Fax +1 630 482 2956
www.asconcorp.com
info@asconcorp.com

DISTRIBUTORS

ARGENTINA

Meditecna s.r.l.

Phone +5411 4585 7005
Fax +5411 4585 3434

AUSTRALIA

Onetemp PTY - Ipa Industrial Pyrometer (Aust) PTY.LTD

Phone +61 8 8352 3688
Fax +61 8 8352 2873

FINLAND & ESTONIA

Tim-Tool oy

Phone +358 50 501 2000
Fax +358 9 50 55 144

GERMANY

Mesa Industrie Elektronik GMBH

Phone +49 2365 915 220
Fax +49 2365 915 225

GREECE

Control System

Phone +30 31 521 055-6
Fax +30 31 515 495

Branch Office

Phone +30 1 646 6276
Fax +30 1 646 6862

HOLLAND

Tempcontrol IEP B.V.

Phone +31 70 3476431
Fax +31 70 3825516

POLAND

ASCON POLSKA Sp. z o.o.

Phone +48 34 35 33 619
Fax +48 34 35 33 884

PORTUGAL

Regiquipamentos LDA

Phone +351 21 989 0738
Fax +351 21 989 0739

SPAIN

Interbil S.L.

Phone +34 94 453 50 78
Fax +34 94 453 51 45

Branch Office

Phone +34 93 311 98 11
Fax +34 93 311 93 65
Phone +34 91 656 04 71
Fax +34 91 677 21 26

SWITZERLAND

Controltherm GMBH

Phone +41 1 954 37 77
Fax +41 1 954 37 78

TURKEY

Kontrol Sistemleri LTD

Phone +90 216 302 19 70-71
Fax +90 216 302 19 72

UNITED KINGDOM

Eukero Controls LTD

Phone +44 20 8568 4664
Fax +44 20 8568 4115

CONFIGURATION PARAMETERS TABLES

Parameter	Variable	Default value	User settings	Notes
Con.1	Configuration Code	9999		
Con.2	Second (Alarms) Configuration Code	0000		
LFr9	Line Frequency	60		
Unit	Engineering Units	NONE		
in.1dd	Decimal Point	0		
tF iL 1	Input 1 Filter	OFF		
in.1Lo	Input Low Range	0		
in.1H 1	Input High Range	99999		
in 1Cn	Input 1 Conditioning	NONE		
CutE 1	Input 1 Cut – Off square root	0		
in.1Sh	Input 1 Shift	0FF		
in2.5t	Input2 Type	NONE		
in.2dd	Input 2 Decimal Point	0		
tF iL2	Input 2 Low Range	0		

Parameter	Variable	Default value	User settings	Notes
in.2Hi	Input 2 High Range	99999		
in.2Cn	Input 2 Conditioning	NONE		
Cut 2	Input 2 Cut – Off square root	0		
in.2Sh	Input 2 Shift	NONE		
C in	Calculated value selection	NONE		
C in.Lo	Cin input Low Range	0		
C in.Hi	Cin input High Range	99999		
C in.dd	Cin Decimal Point	0		
AO.Src	Analog Out Signal	NONE		
AO.tYP	Analog Out Type	0 - 20		
AO.Lo	Analog Out Low Range	0		
AO.Hi	Analog Out High Range	100		
IL 1	Digital Input 1 Configuration	NONE		
IL2	Digital Input 2 Configuration	NONE		
IL3	Digital Input 3 Configuration	NONE		
Prot	Communications Protocol	MBUS		
baud	Baud Rate	9600		
Par.Y	Parity	NONE		

Parameter	Variable	Default value	User settings	Notes
Addr	Serial Communications Address	247		
CodE 1	Full Access Password	11		
CodE2	Sensor Cal & Par Menu Access Password	22		
CodE3	Sensor Cal Access Password	33		
AL.1Sr	AL1 Source	IN1		
AL.2Sr	AL2 Source	IN1		
AL.3Sr	AL3 Source	IN1		
AL.4Sr	AL4 Source	IN1		
AL.1OP	AL1 Out	NONE		
AL.2OP	AL2 Out	NONE		
AL.3OP	AL3 Out	NONE		
AL.4OP	AL4 Out	NONE		
AL.1Lb	AL1 Latching/Blocking	NONE		
AL.2Lb	AL2 Latching/Blocking	NONE		
AL.3Lb	AL3 Latching/Blocking	NONE		
AL.4Lb	AL4 Latching/Blocking	NONE		
ALnSr	Alarm Reference Source	INT		
OP.1d	OP1 Action	NORM		norm/InV

Parameter	Variable	Default value	User settings	Notes
OP.2A	OP2 Action	NORM		norm/InV
OP.3A	OP3 Action	NORM		norm/InV
OP.4A	OP4 Action	NORM		norm/InV
SH.CAL	High calibration value	80		
CALMd	Calibration Mode	ZERO		
SGCAL	User Calibration Menu Enable	ON		
rArEN	Tare Menu Enable	ON		
rArEE	Tare value Editing Enable	ON		
FAct	Factory calibration	OFF		
SEt.t	Set tare	NO		
CLEAr	Clear tare value	NO		
Zroc	Zero calibration	NO		
hiCAL	Span calibration	NO		
AL.1SP	Alarm_1 Threshold	0		
AL.2SP	Alarm_2 Threshold	0		
AL.3SP	Alarm_3 Threshold	0		
AL.4SP	Alarm_4 Threshold	0		
ALrEF	Alarm internal reference value	0		

Parameter	Variable	Default value	User settings	Notes
AL.1HY	Alarm_1 Hysteresis	0.5		
AL.2HY	Alarm_2 Hysteresis	0.5		
AL.3HY	Alarm_3 Hysteresis	0.5		
AL.4HY	Alarm_4 Hysteresis	0.5		
AL.1d	Alarm_1 Delay	0		
AL.2d	Alarm_2 Delay	0		
AL.3d	Alarm_3 Delay	0		
AL.4d	Alarm_4 Delay	0		
FiLtd	Filter display	2.0		
rESd	Resolution diplay	1		
HId.TM	Hold Time	5		
dEF.SH	Default visualization in manual mode	IN1		
t iME.S	Alternate Time	5		